

Application Bulletin

ORP Measurements

ORP (Oxidation-Reduction or redox Potential) measurement is used to indicate the presence of oxidizing or reducing conditions in water. In pure water treatment, ORP is most commonly used to assure removal of chlorine or other oxidizing agent ahead of membranes or deionization resins that could be damaged by oxidation. It can warn if the bisulfite feed or carbon bed is not properly removing the chlorine. ORP is also used in other process and wastewater applications.

	Oxidizing Agents	Reducing Agents
Example chemicals	Chlorine, hypochlorite, peroxide, ozone, permanganate	Bisulfites, activated carbon
Typical reaction	Cl_2 + 2e ⁻ \rightarrow 2Cl ⁻	SO_3^{2-} + H ₂ O \rightarrow
		SO ₄ ²⁻ + 2H ⁺ + 2e ⁻
Electrochemical response	accepts electrons, raises ORP	donates electrons, lowers ORP

ORP Significance

The correlation between the concentration of chlorine or other oxidizing or reducing material and ORP varies. ORP is logarithmically related to concentration, however, the variables of pH, temperature and other oxidizing or reducing materials in the water can cause ORP response to shift significantly. For this reason there is no reliable conversion from ORP in millivolts to concentration in parts per million or billion.

In moving from an oxidizing to a reducing condition with extremely small (parts per billion) concentration changes, the ORP typically drops several hundred millivolts. It is very sensitive in detecting the change and is therefore quite useful as a go/no-go alarm parameter. In alarm applications, the exact setpoint value is usually not critical. However, where ORP is used to control bisulfite feed, more precision is needed in establishing the control point. A titration curve illustrates ORP response and the considerations in establishing a setpoint.


An ORP titration curve of dechlorination shows the type of response that would be expected for treatment of an off-line grab sample. Chlorinated water in this example gives an ORP of over 700 mV on the left. As small amounts of reducing bisulfite solution are added, the ORP drops in a very non-linear fashion. As the chlorine is all reacted and an excess of bisulfite accummulates, the response reaches a plateau near 350 mV to the right. It is important to establish the setpoint somewhat above the plateau to prevent wasting bisulfite or causing false alarms. The sensitivity of this measurement is apparent from the steep portion of the curve which is the transition from oxidizing to reducing conditions. Continuous processes are controlled to operate near a single point on such a curve.

NOTE: This is only an example titration curve. The curve for a specific installation may be shifted significantly from these millivolt values but the basic shape will be similar for the dechlorination reaction. Online experience is necessary at startup to establish the particular millivolt operating range and setpoint for an application. 1

The best practice to determine a setpoint for control is to use a colorimetric or other sensitive test for chlorine or bisulfite concentration as a reference. The ORP existing at the time the desired concentration is reached is an appropriate setpoint value. Test kits for these materials are readily available.

ORP sensors and instrumentation are very similar to pH. However, the measuring electrode is an inert metalplatinum or gold. The metal electrode merely picks up the ORP millivolt signal – the solution's tendency to contribute or remove electrons from its surface. The reference electrode completes the circuit and adds in its own (nearly constant) potential. The instrument measures the combined potential and displays it directly in millivolts.

Typical ORP Titration Curve for Dechlorination

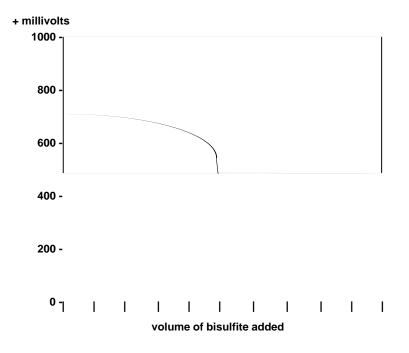

There is generally no calibration of sensors. Direct, absolute millivolts are the usual unit of measure. (Because ORP instruments are typically pH instruments operating in a millivolt mode, calibration is possible which yields a relative millivolt reading. ORP standard solutions are available but they have fairly wide tolerances under process conditions. ORP standards are used primarily for verification of electrode response rather than calibration.)

2

There is no temperature compensation with ORP instrumentation as each oxidation-reduction reaction has somewhat different temperature characteristics and most processes using ORP have fairly stable temperature.

Other Applications

ORP has excellent sensitivity in low concentrations (ppb ranges) where it is desired to remove an oxidizing or reducing material. At higher concentrations, such as to establish a residual chlorine concentration of several parts per million, the sensitivity for the particular application should be examined by actual titrations of samples under various operating conditions. In some cases, a residual chlorine analyzer may provide better sensitivity.

Plating Wastewater treatment uses ORP to control treatment of plating rines waters containing chromium or cyanide. Chromium must be reduced under acidic conditions (usually with bisulfite) to the form that can be precipitated and removed when the pH is raised again. Cyanide must be oxidized (usually with chlorine) under alkaline conditions to produce harmless bicarbonate and nitrogen. For further information on these processes contact Mettler-Toledo Thornton application support.

Further Reading

- 1. `ASTM Test Method D1498, ASTM, Conshohocken, PA.
- 2. Gray and Marshall, "ORP Measurement in Water and Wastewater," Ultrapure Water Journal, Sept/Oct 1993.
- 3. Liptak, ed, Instrument Engineers' Handbook--Process Control, Chilton, Chapter 8.15, 1985.
- 4. Shinskey, pH and plon Control in Process and Waste Streams, Wiley 1973.

For the most current product information visit: **WWW.thorntoninc.com**

Mettler-Toledo Thornton, Inc. 36 Middlesex Turnpike Bedford, MA 01730 USA Telephone: +1-781-301-8600 Toll-Free: 1-800-510-PURE Customer/Technical Service Telephone: +1-781-301-8690 Toll-Free: 1-800-642-4418 Cust Service Fax: +1-781-271-0214 Tech Service Fax: +1-781-271-0675

[®] Mettler-Toledo Thornton, Inc. – Subject to Technical Changes

email: info@thorntoninc.com www.thorntoninc.com

Created 01/98 Updated logo & address 09/03